

Figure 1


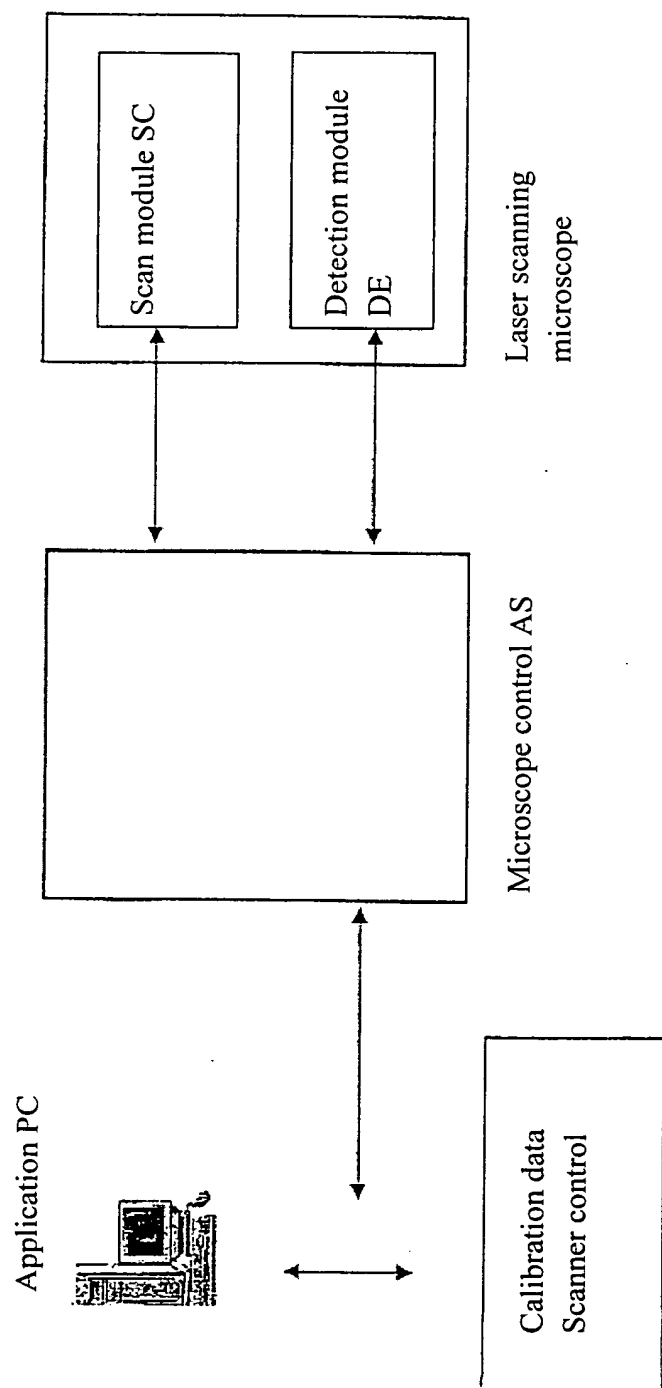


Figure 2

a)

Correlation of partial images of the forward or back scan in the x scanner direction (example cross-grid sample, for example 20 μm grid):

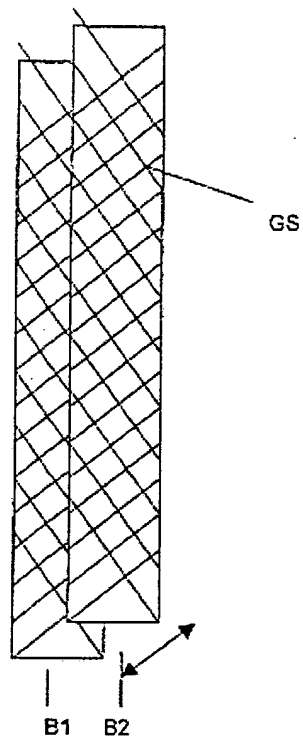

b)

Correlation in the y scanner direction:

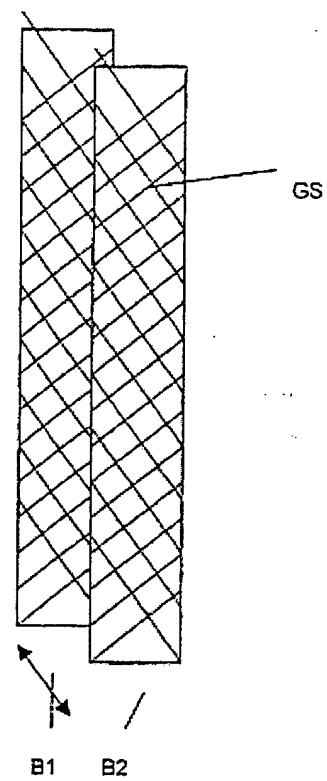


Figure 3

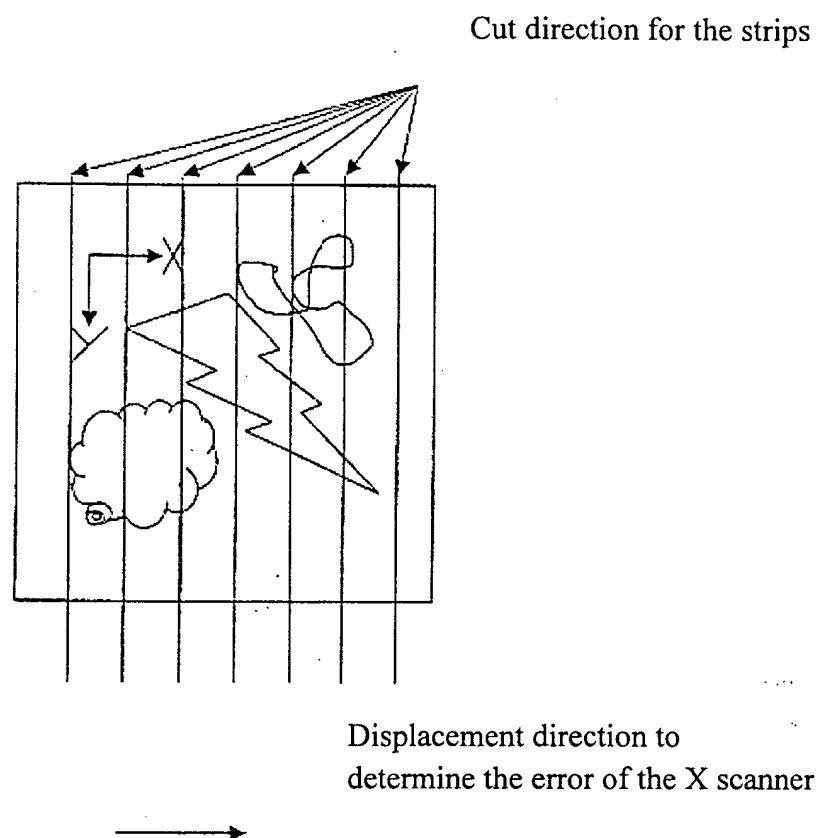


Figure 4

Cut direction for the strips

